

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.


Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**



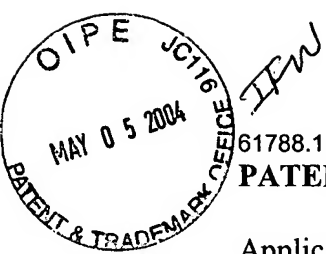

61788.1

PATENT

13595US

**IN THE UNITED STATES PATENT AND TRADEMARK OFFICE**

Applicant: Behrenbruch, et al. Examiner: To be assigned

Serial No.: 10/756,953 Group Art Unit: 2882

Filed: January 13, 2004

For: Improvements in or Relating to Dynamic Medical Imaging

Customer No.:



23719

PATENT TRADEMARK OFFICE

Kalow & Springut LLP  
488 Madison Avenue, 19th Floor  
New York, New York 10022

May 3, 2004

Commissioner for Patents  
P.O. Box 1450  
Alexandria, VA 22313-1450**TRANSMITTAL OF CERTIFIED COPY OF PRIORITY DOCUMENT**

S I R:

Enclosed is a certified copy of the priority document, U.K. 0300921.4, for the above-identified application. No fee is believed to be due in connection with this transmittal. If any fee is due, please charge Deposit Account No. 11-0171 for such sum accordingly.

No other fee is believed to be due with this order. If any additional fee is due, or if an overpayment has been made, please charge or credit Deposit Account No. 11-0171 for such sum.

Respectfully submitted,

William D. Schmidt

Registration No.: 39,492

Attorney for Applicant

Kalow & Springut LLP  
(212) 813-1600**Certificate of Mailing Under 37 C.F.R. 1.8**

I hereby certify that this correspondence is being deposited on the date shown below with the United States Postal Service as first class mail with sufficient postage in an envelope addressed to: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.

  
(Signature)Sylvia Goral  
(Printed Name of Person Signing Certificate)May 3, 2004  
(Date)





INVESTOR IN PEOPLE

The Patent Office  
Concept House  
Cardiff Road  
Newport  
South Wales  
NP10 8QQ

I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation & Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with the patent application identified therein.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.

In accordance with the rules, the words "public limited company" may be replaced by p.l.c., plc, P.L.C. or PLC.

Re-registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.


Signed 

Dated 4 March 2004



# Patents Form 1/77

Patents Act 1977  
(Rule 16)

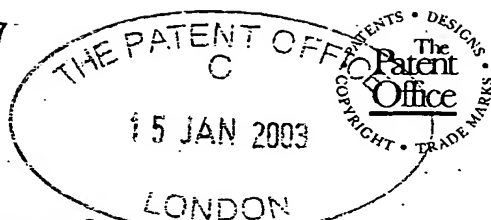

1/77  
16JAN03 9777352-2 D00192  
P01/7700 0:00-0300921.4

## Request for grant of a patent

(See the notes on the back of this form. You can also get an explanatory leaflet from the Patent Office to help you fill in this form)

The Patent Office

Cardiff Road  
Newport  
South Wales  
NP10 8QQ

|   |   |   |  |
|---|---|---|--|
| 1. Your reference   | N.87371 MN  |   |  |
| 2. Patent application number<br>(The Patent Office will fill in this part)  | 0300921.4   |   | 15 JAN 2003                            |
| 3. Full name, address and postcode of the or of each applicant (underline all surnames)   | MIRADA SOLUTIONS LIMITED<br>Oxford Centre for Innovation<br>Mill Street<br>Oxford OX2 0JX<br>United Kingdom |   |  |
| Patents ADP number (if you know it)   |   |   |  |
| If the applicant is a corporate body, give the country/state of its incorporation   | GB  |   |  |
| 4. Title of the invention   | IMPROVEMENTS IN OR RELATING TO DYNAMIC MEDICAL IMAGING  |   |  |
| 5. Name of your agent (if you have one)   | J.A. KEMP & CO.   |   |  |
| "Address for service" in the United Kingdom to which all correspondence should be sent (including the postcode)   | 14 South Square<br>Gray's Inn<br>London<br>WC1R 5JJ   |   |  |
| Patents ADP number (if you know it)   |   |   |  |
| 6. If you are declaring priority from one or more earlier patent applications, give the country and the date of filing of the or of each of these earlier applications and (if you know it) the or each application number  | Country   | Priority application number<br>(if you know it) | Date of filing<br>(day / month / year) |
| 7. If this application is divided or otherwise derived from an earlier UK application, give the number and the filing date of the earlier application   | Number of earlier application   |   | Date of filing<br>(day / month / year) |
| 8. Is a statement of inventorship and of right to grant of a patent required in support of this request? (Answer 'Yes' if:<br>a) any applicant named in part 3 is not an inventor, or<br>b) there is an inventor who is not named as an applicant, or<br>c) any named applicant is a corporate body.<br>See note (d)) | Yes   |   |  |

## Patents Form 1/77

9. Enter the number of sheets for any of the following items you are filing with this form. Do not count copies of the same document

Continuation sheets of this form

|             |                 |
|-------------|-----------------|
| Description | 9               |
| Claim(s)    | 3               |
| Abstract    | 1               |
| Drawing(s)  | 5 + 5 <i>Rm</i> |

10. If you are also filing any of the following, state how many against each item.

Priority documents

Translations of priority documents

Statement of inventorship and right to grant of a patent (*Patents Form 7/77*)

Request for preliminary examination and search (*Patents Form 9/77*) 1

Request for substantive examination (*Patents Form 10/77*)

Any other documents (*please specify*)

11. I/We request the grant of a patent on the basis of this application.

Signature

*J.A. Kemp*

Date 15 January 2003

J.A. KEMP & CO.

12. Name and daytime telephone number of person to contact in the United Kingdom

NICHOLLS, Michael John  
020 7405 3292

### Warning

*After an application for a patent has been filed, the Comptroller of the Patent Office will consider whether publication or communication of the invention should be prohibited or restricted under Section 22 of the Patents Act 1977. You will be informed if it is necessary to prohibit or restrict your invention in this way. Furthermore, if you live in the United Kingdom, Section 23 of the Patents Act 1977 stops you from applying for a patent abroad without first getting written permission from the Patent Office unless an application has been filed at least 6 weeks beforehand in the United Kingdom for a patent for the same invention and either no direction prohibiting publication or communication has been given, or any such direction has been revoked.*

### Notes

- If you need help to fill in this form or you have any questions, please contact the Patent Office on 08459 500505.*
- Write your answers in capital letters using black ink or you may type them.*
- If there is not enough space for all the relevant details on any part of this form, please continue on a separate sheet of paper and write "see continuation sheet" in the relevant part(s). Any continuation sheet should be attached to this form.*
- If you have answered 'Yes' Patents Form 7/77 will need to be filed.*
- Once you have filled in the form you must remember to sign and date it.*
- For details of the fee and ways to pay please contact the Patent Office.*



IMPROVEMENTS IN OR RELATING TO  
DYNAMIC MEDICAL IMAGING

The present invention relates to dynamic medical imaging, that is to say the  
5 acquisition of a plurality of time separated images of a subject in order to reveal  
some aspect of the medical condition of the subject.

Medical imaging is a technology that has evolved substantially over the past  
few decades with an increasing diversity of modalities - Magnetic Resonance  
Imaging (MRI), Computed Tomography (CT), Nuclear Medicine (NM) and Positron  
10 Emission Tomography (PET) - to name but a few. Although the traditional notion of  
medical imaging involves the acquisition of a "static" image that captures the  
anatomy of an organ/region of the body, increasingly the use of more sophisticated  
imaging techniques allows dynamic studies to be made which provide a temporal  
sequence of images which can characterise physiological or pathophysiological  
15 information.

Both static and dynamic medical imaging may involve the use of an imaging  
technique to increase selectively the contrast of a certain region in the image (e.g. on  
the basis of that region's structure or physiological state). For example, one may  
inject into a patient a compound which has a biophysical, molecular, genetic or  
20 cellular affinity for a particular organ, disease, state or physiological process. Such  
contrast agents are selected to have a property that provides enhanced information to  
a given imaging modality by altering imaging conditions (normally by altering the  
contrast) to reflect the behaviour of the compound in the body. This may be  
achieved via increased X-ray attenuation a localised site (e.g. for CT/X-ray), altered  
25 paramagnetic properties (e.g. for MRI) or the use of a radioisotope for nuclear  
medicine/PET. Such contrast agents are well-known for many imaging modalities.  
In some cases a technique may be used to create a contrast enhancement which does  
not rely on an injected contrast agent, for instance the use of "black blood" or "white  
blood" in magnetic resonance (MR) imaging (where specific pulse sequences are  
30 used to change the magnetic saturation of the blood and thus its appearance in the

image), or tagged MR sequences which alter the magnetic behaviour of particular tissue or fluid. An injected contrast agent, or a tissue or fluid with altered behaviour, may all be regarded as "imaging agents".

Analysis of the behaviour of an imaging agent through imaging typically involves an acquisition process that takes many "snapshots" of the organ/region/body over time in order to capture the time-varying behaviour, e.g. distribution, of the agent and hence capture a specific biological state (disease, condition, physiological phenomenon, etc.). As the speed and digital nature of medical imaging evolves, this acquisition data can have tremendous temporal resolution and results in large quantities of data.

Additionally, there is a growing interest in not only imaging a particular physiological phenomenon to characterise a disease or condition, but also the in vivo assessment of the change in disease in response to therapy. This therapy may be surgical, pharmacological/genetic or radiotherapeutic in nature. Whether for diagnosis or treatment assessment purposes, dynamic imaging is a powerful clinical tool and has not only altered the landscape of medical imaging but has also made substantial inroads into drug discovery and animal applications.

Irrespective of the application, dynamic imaging with an imaging agent requires a temporal (multiple time epoch) acquisition during which the behaviour of the imaging agent is characterised. Sometimes this characterisation involves known physiological, cellular or genetic models that may have arbitrary interaction complexity. Sometimes this characterisation is performed using mathematical or statistical models that abstract true physiological meaning but which may enable certain parameters to be calculated which indicate the behaviour of the imaging agent and hence provide diagnostic information.

A patient may need to spend considerable time in an imaging device in order to acquire an image sequence. During this time, a patient may move - either due to natural bodily motion (respiration, "physiological tremor", etc) or as part of a symptom of disease (e.g. lack of motor control by an Alzheimer's patient). This motion necessarily corrupts the temporal accuracy of the imaging process, making it

difficult to compare and, more critically, analyse individual regions of the imaging process.

Algorithms and clinical methods to address motion have long been a focus of research in medical imaging. Various techniques for motion correction, often  
5 involving registering images together to match corresponding locations in the image to each other, have been proposed, see for example WO 00/57361 and D. Rueckert, C. Hayes, C. Studholme, P. Summers, M. Leach, D. Hawkes, "Non-Rigid Registration of Breast MR Images Using Mutual Information", in Proc. MCCA  
10 1152, ISBN 3-540-65136-5, Springer Verlag. However such methods have failed to address the following issues:

- 1) The validity of the motion correction.
- 2) Feedback to the user about the quality of the motion correction in a region of interest.
- 15 3) Feedback to the motion correction process itself regarding correction quality and analytical usefulness of the motion correction data.

In virtually all dynamic imaging studies that involve an imaging agent, the behaviour of the agent can be mathematically characterised at some level or another. In the most simplistic fashion the behaviour of an imaging agent such as an injected  
20 compound may be analysed using a model of "uptake" and possibly subsequent "wash out", which may be linear or non-linear in nature. In more sophisticated instances, biophysical and pharmacokinetic understanding enables an imaging agent to be analysed using complex models that describe many different phases of behaviour and interaction. This is illustrated in Figure 1 of the accompanying  
25 drawings, which show a dynamic MR imaging sequence of the breast as a contrast agent is injected. The left breast (on the right in the displayed coronal slice) is the region of interest, where the suspicious area needs clinical investigation using contrast-enhanced MRI. Figure 1(a) illustrates the baseline image, that is to say with no imaging agent. Figure 1(b) schematically represents the injection of contrast  
30 agent and the enhancement of the breast starts in Figure 1(c), continues in Figure 1(d)

and finishes later in Figure 1(e) with high enhancement of the breast. Figure 1(f) represents the amount of image enhancement of the circled region in the image of Figures 1 (a),(c), (d) and (e) plotted as a function of time. This can be fitted to the expected mathematical model of the uptake and washout rates of this contrast agent and from the fitted curve a value for the uptake rate and washout rate can be calculated. These values can be used to characterise the tissue in the circled region as cancerous or normal.

However, Figure 1 illustrates schematically the ideal case where there is no patient movement. If the patient moves, this adds noise or corrupts the imaging information that is used for this dynamic analysis. Without motion correction, it can be understood that this will change the values for apparent image enhancement at any particular part of the breast (because the values will not be referring to the same part of the breast before and after movement). Thus if patient motion occurs it is no longer possible to analyse accurately the temporal characteristics of an imaging process.

Figure 2 illustrates two sequences of images, a first in which motion is not corrected and a second in which motion is corrected. In the first sequence Figure 2(a) is a baseline (i.e. before injection of contrast agent) magnetic resonance image of another breast clinical case. Figure 2(b) shows the image after a gadolinium contrast agent has been injected. An easy way to judge the amount of enhancement, and thus isolate the tumourous region, is to subtract the two images of Figures 2(a) and 2(b). This results in the subtraction image of Figure 2(c). Unfortunately because the patient moved between the pre-contrast and post-contrast images of Figures 2(a) and 2(b), the subtraction image of Figure 2(c) contains many artefacts that suggest enhancement, but are in fact erroneous. One of the known motion correction techniques of registering the pre- and post-contrast images to each other can be used to find the motion field in the image. A suitable technique is disclosed in WO 00/57361 (herein incorporated by reference). The resulting motion field is shown in Figure 2(d). It can be seen that there is significant motion in the right-hand part of the breast, but no motion in the left-hand part. The post-contrast image can be

motion corrected to remove the movement resulting in the corrected image of Figure 2(e), and then this is subtracted from the pre-contrast image of Figure 2(a). The corrected subtraction image is shown in Figure 2(f) and it can be seen that many motion artefacts have been removed (for example the highly visible artefacts around the edge of the breast in Figure 2(c)), and the region corresponding to contrast enhancement (for instance tumours) within the breast is more clearly visible.

Although such motion correction techniques are useful, they are often regarded with suspicion by clinicians. This is especially true of non-rigid, or deformable, corrections where clinicians worry that the changes introduced by the motion correction may disguise clinically significant features. This has lead to a slow take-up in practice of the advantages given by registration techniques.

The present invention provides a method of dynamic medical imaging in which the expected temporal characteristics of the imaging process, e.g. the model of behaviour of the imaging agent, is used to optimise a motion correction process, such as one of the known methods of registration, and to provide feedback to the user as to the quality of motion correction.

Thus the knowledge about the temporal behaviour of the imaged region can be used not only in the conventional diagnosis, but also to validate the motion correction. Further, if the motion correction is found by this method to be poor, it provides a way of identifying regions within the subject where the motion correction is poor, allowing them to be processed further, for instance using different parameters in the motion correction method. The invention also provides quality-control information to the user of the dynamic/temporal medical imaging study.

In more detail the present invention provides a method of dynamic medical imaging comprising the steps of:-

- obtaining a plurality of time separated images of the subject;
- registering the plurality of time separated images together to match corresponding locations in the images to each other;
- measuring from the registered images the temporal behaviour of an imaged region at a location in the subject; and

comparing the measured temporal behaviour with a model of the expected temporal behaviour of the imaged region to determine the level of agreement therebetween as a measure of the quality of the registration of the time separated images.

5        Thus the expected behaviour of the imaged region is used to measure the quality of the registration.

The images may be acquired in a process involving the use of an imaging agent. The imaging agent may be the subject's own tissue or fluid or a contrast agent which is administered to the subject as mentioned above.

10       The level of agreement between the measured and expected temporal behaviour may be displayed to the user, for instance overlying an image of the subject, for example as a colour wash with different colours or intensities indicating the level of agreement.

The method may further include the step of re-executing the image registration in regions of the image where the level of agreement is poor. This may be achieved by using different parameters, such as using a different resolution, different scale or different sized search windows in the registration process.

The model may be a temporal model of the take-up and wash-out of an imaging agent and the subject of the imaging process may be a living human, animal  
20 or plant.

The technique is applicable to any dynamic imaging technique such as magnetic resonance imaging, computed tomography, positron emission tomography, nuclear medicine, ultrasound, x-ray and optical imaging.

The invention may be embodied as a computer program comprising program  
25 code means for executing the registration, measurement and comparison steps on a programmed computer, and the invention extends to a computer readable storage medium carrying such a program and to a computer system programmed to execute the method.

The invention will be further described by way of example with reference to  
30 the accompanying drawings, in which:-

Figure 1(a) to (g) illustrate schematically the prior art concept of dynamic imaging using an imaging agent and the process of analysis;

Figures 2(a) to (f) illustrate two sequences of MR images of a contrast-enhanced breast illustrating the techniques of motion correction;

5        Figure 3(a) to (f) illustrates in similar fashion to Figure 1 the verification of the motion correction using the model of imaging agent behaviour;

Figure 4 illustrates a schematic flow diagram of the process of one embodiment of the invention; and

10        Figure 5 illustrates the application of one embodiment of the invention to a recalculation of motion correction.

Referring to Figures 3 and 4 an embodiment of the invention based on the MR imaging technique of Figure 1 will be described. Firstly in step 400 of Figure 4 a dynamic image sequence is acquired from a patient 42 using an imaging apparatus 46 during injection of an imaging agent 44 such as Gadolinium DTPA (Diethyline  
15    Triamine Pentaacetic Acid). The sequence is illustrated schematically in Figure 3(a). It is assumed that there is some patient head motion in the imaging sequence. In step 402 a registration process is carried out to correct the patient motion. The technique may be that described in WO 00/57361. Then the temporal behaviour of the enhancement in a particular part of the image is measured in step 404 - the values of  
20    enhancement against time are plotted as crosses in Figure 3(b). The continuous line in Figure 3(b) illustrates the fitted model, for example in this case the fitted model of the enhancement rate for this imaging agent. Comparing this with Figure 1(g) it can be seen that the fit is quite poor, this being caused by patient movement. Figure 3(c) illustrates the numerical fitting error calculated in step 406, i.e. the difference  
25    between the value of the data point and the fitted curve.

Incidentally, it is possible to apply steps 404 and 406 before applying any image registration algorithm, i.e. before step 402.

The amount of error is displayed in step 407, for example as an overlay whose colour and/or intensity indicate the level of error, or as lines whose length  
30    indicate the amount of error. This display gives the user an indication of the quality

of the motion correction. If the fit is very poor, this is taken to indicate that there is a substantial degree of patient motion. On the other hand, if the fit is good, this indicates that the patient has not moved much. Obviously there may be different qualities of fit for different parts of the image where some parts of the subject moves but not others.

In this embodiment in regions of the image where the fit is not good enough as indicated by step 408, the motion correction is re-executed in step 410 and the model of the temporal behaviour of the imaging agent is fitted again to the data. The motion correction can be done by any of the following, for example:

- a) addition of extra control points of a parametric transformation in areas or misalignment as shown in Figure 5;
- b) locally loosening stiffness and regularisation constraints in areas of misalignment in the computation of a displacement field;
- c) locally changing the scale of the displacement field characteristics; and
- d) locally changing the characteristics of local block (size, search, step, etc.) in a block matching technique.

Steps 406, 408 and 410 are repeated iteratively until the residual error is acceptable or at a minimum. This is illustrated in Figures 3(d) and (e), where Figure 3(e) illustrates the corrected data points and the much better fit to the model curve. Figure 3(f) illustrates the residual error, now much lower than in Figure 3(c). When the fit is good enough the newly corrected motion image can be displayed in step 412 and the diagnostic parameters such as the wash-in rate and wash-out rate can be calculated taking into account the improved motion correction.

Thus the present invention combines the knowledge about the temporal behaviour of the imaging agent with the motion correction process in order not only to improve the motion correction process and give an indication of its quality, but also to produce ultimately a better motion corrected image which the temporal behaviour model fits, thus allowing a calculation of the diagnostic parameters even in regions of high patient motion.

The imaging agents usable with the present invention are any of those



suitable for magnet resonance imaging, computed tomography, positron emission tomography, single photon emission computed tomography, nuclear medicine, ultrasound, x-ray (including angiography) and optical imaging, and include ligands/chelates tagged to paramagnetic compounds (for MRI), radio-labelled  
5 tracers/radio pharmaceuticals or nuclear medicine, ionic radiation attenuators for CT and x-ray, receptor-specific imaging agents for cellular behaviour and interactions, genetic markers (radio-labelled, luciferase-labelled etc), blood pool agents and vascular imaging agents.

The invention can be applied to two-dimensional or three-dimensional  
10 imaging processes.

CLAIMS

1. A method of dynamic medical imaging comprising the steps of:-  
obtaining a plurality of time separated images of the subject;  
5 registering the plurality of time separated images together to match  
corresponding locations in the images to each other;  
measuring from the registered images the temporal behaviour of an imaged  
region at a location in the subject; and  
comparing the measured temporal behaviour with a model of the expected  
10 temporal behaviour of the imaged region to determine the level of agreement  
therebetween as a measure of the quality of the registration of the time separated  
images.
2. A method according to claim 1 wherein obtaining the images involves the  
15 use of an imaging agent and said model is a model of the temporal behaviour of the  
imaging agent.
3. A method according to claim 2 wherein the imaging agent is a  
contrast agent.  
20
4. A method according to any one of the preceding claims wherein the  
level of agreement between the measured temporal behaviour and the expected  
temporal behaviour is displayed.
- 25 5. A method according to claim 4 wherein the level of agreement is  
displayed overlying an image of the subject.
6. A method according to any one of the preceding claims further  
comprising re-executing the step of registering the plurality of time separated images  
30 together in imaged regions where the level of agreement is poor.

7. A method according to claim 6 wherein the registration uses a parameterised process and is re-executed using different registration parameters.

5 8. A method according to claim 6 or 7 wherein the registration is re-executed at a different resolution.

9. A method according to claim 6, 7 or 8 wherein the registration is re-executed at a different scale.

10

10. A method according to claim 6, 7, 8 or 9 wherein the registration comprises searching through a search window defined in one of the images and the registration is re-executed using a different sized search window.

15

11. A method according to any one of the preceding claims wherein the model is a temporal model of the take-up and wash-out of an imaging agent administered to the subject.

12. A method according to any one of the preceding claims wherein the  
20 subject is a living human, animal or plant.

13. A method according to any one of the preceding claims wherein the images are acquired by one of magnetic resonance imaging, computed tomography, positron emission tomography, single photon emission computed tomography,  
25 nuclear medicine, ultrasound, x-ray and optical imaging.

14. A computer program comprising program code means for executing the steps in claim 1 of registering the plurality of time separated images together to match corresponding locations in the images to each other; measuring from the  
30 registered images the temporal behaviour at a location in the subject; and comparing

the measured temporal behaviour to a model of the expected temporal behaviour to determine the level of agreement therebetween as a measure of the quality of the registration of the time separated images.

5        15.     A computer program according to claim 14 further comprising  
program code means for executing the steps of any one of claims 3 to 10.

16.     A computer readable storage medium carrying a computer program  
according to claim 14 or 15.

10

17.     Dynamic medical image processing apparatus adapted to execute the  
steps in claim 1 of registering the plurality of time separated images together to  
match corresponding locations in the images to each other; measuring from the  
registered images the temporal behaviour of the imaging agent at a location in the  
15 subject; and comparing the measured temporal behaviour of the imaging agent to a  
model of the expected temporal behaviour to determine the level of agreement  
therebetween as a measure of the quality of the registration of the time separated  
images.

20        18.     Dynamic medical image processing apparatus according to claim 17,  
further adapted to execute the steps of any one of claims 4 to 11.

25


30

ABSTRACT  
IMPROVEMENTS IN OR RELATING TO  
DYNAMIC MEDICAL IMAGING

5       A method of dynamic medical imaging in which the quality of image  
registration or motion correction between the frames is assessed by examining the  
temporal behaviour of a region of interest through the sequence, and in particular  
how closely the behaviour follows expected behaviour. For a temporal sequence a  
temporal model of the expected behaviour of the region of interest is available and  
10   the quality of fit between the model and the data points from the dynamic imaging  
sequence can be calculated. In image regions of high patient motion the fit will be  
poor, whereas if there is no patient motion the fit will be better. The quality of fit can  
be displayed on the image as an indication of the validity of motion correction, and in  
areas of poor fit the motion correction can be re-executed using different parameters  
15   to try and improve the fit between the behaviour model and the actual data points.  
The invention is applicable to any contrast-enhanced medical imaging technique.




Figure 1

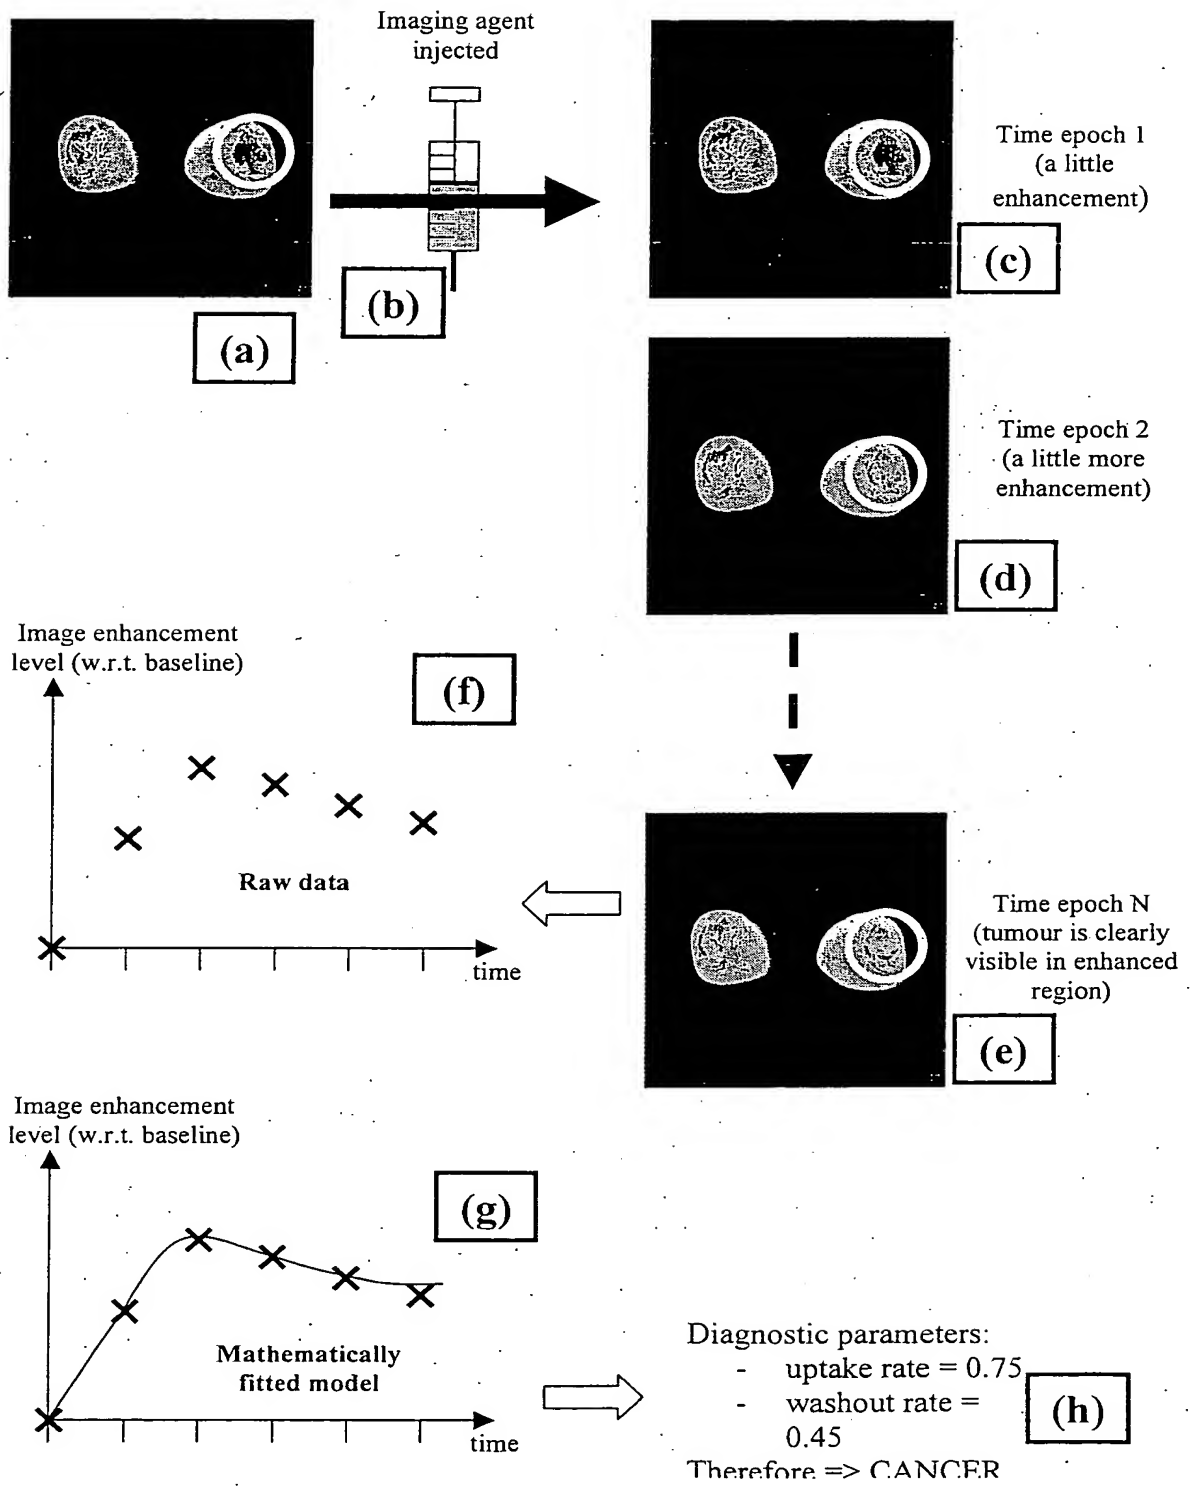





**Figure 2**

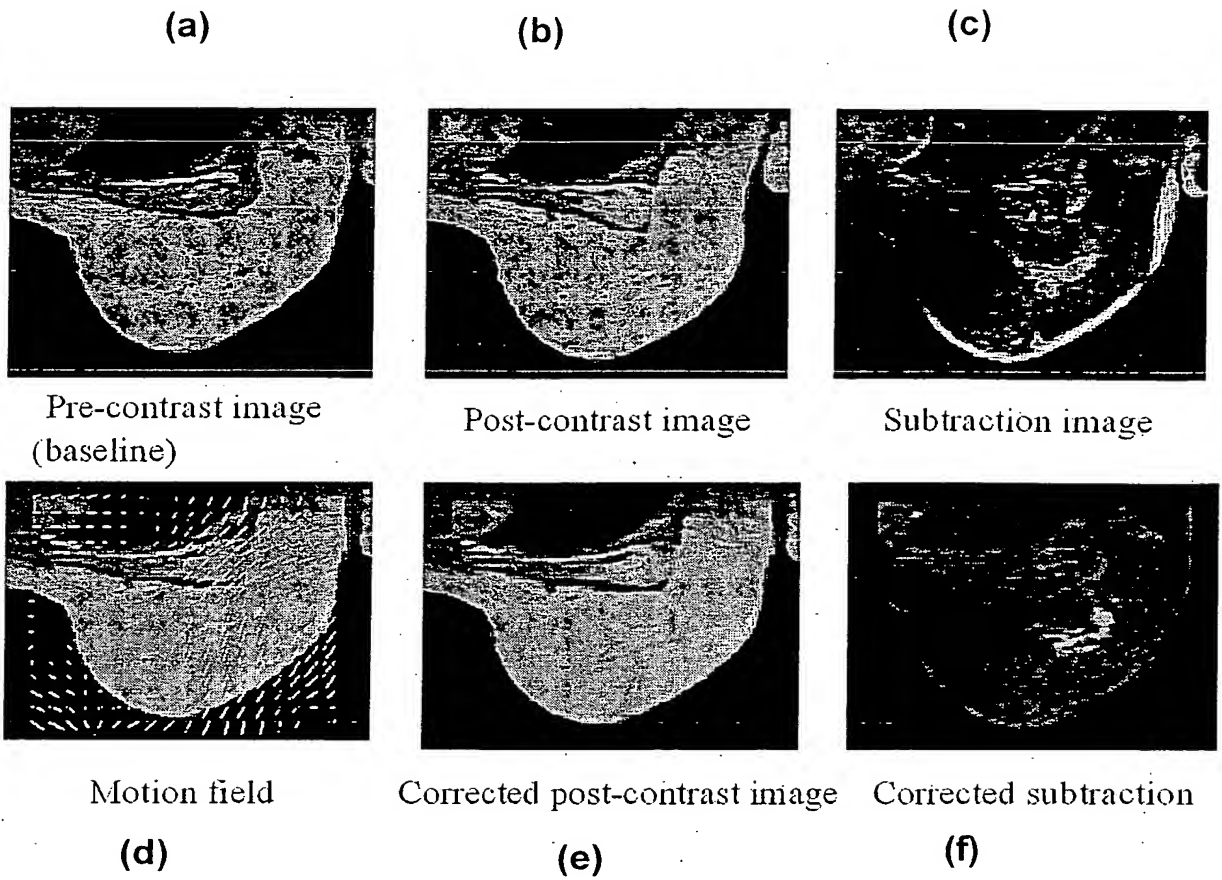



**Figure 3**


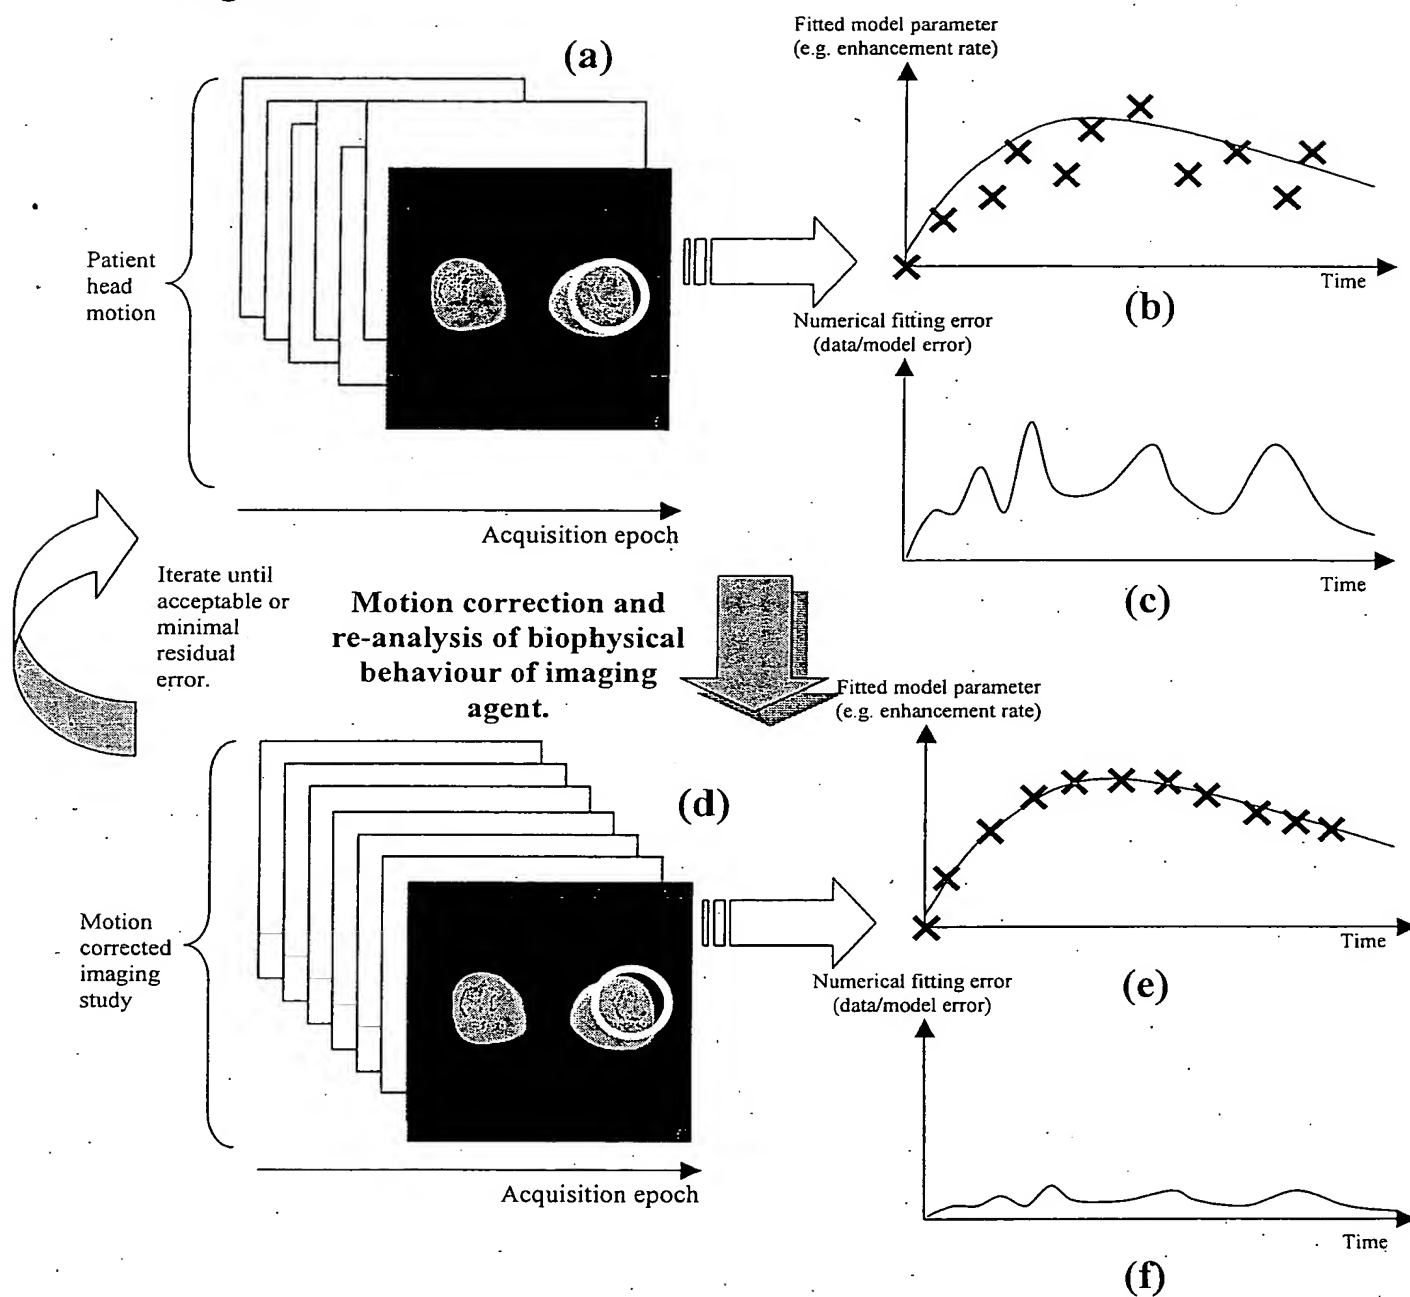




Figure 4



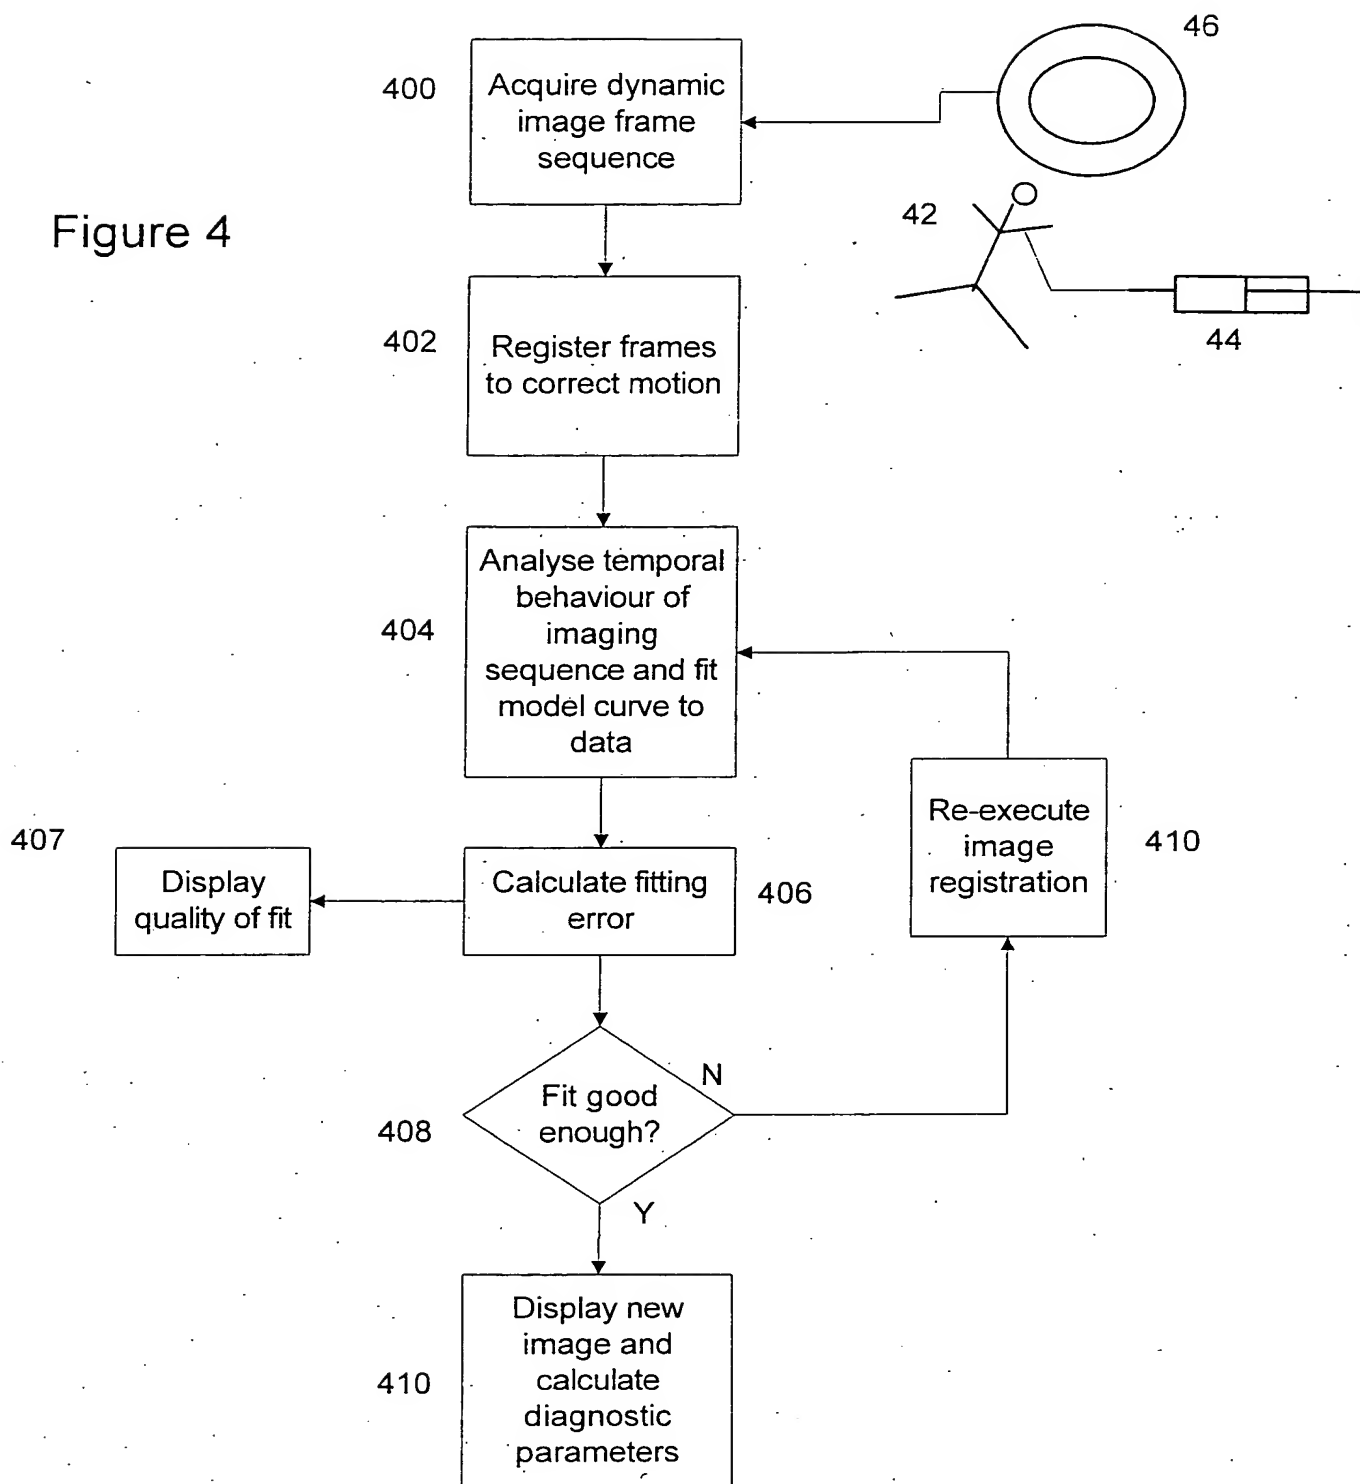

4

4

4

4

Figure 5

